


# Control Program for ISM01

File Selection Settings ComPort Info

not calibrated

Date: 30.07.2006

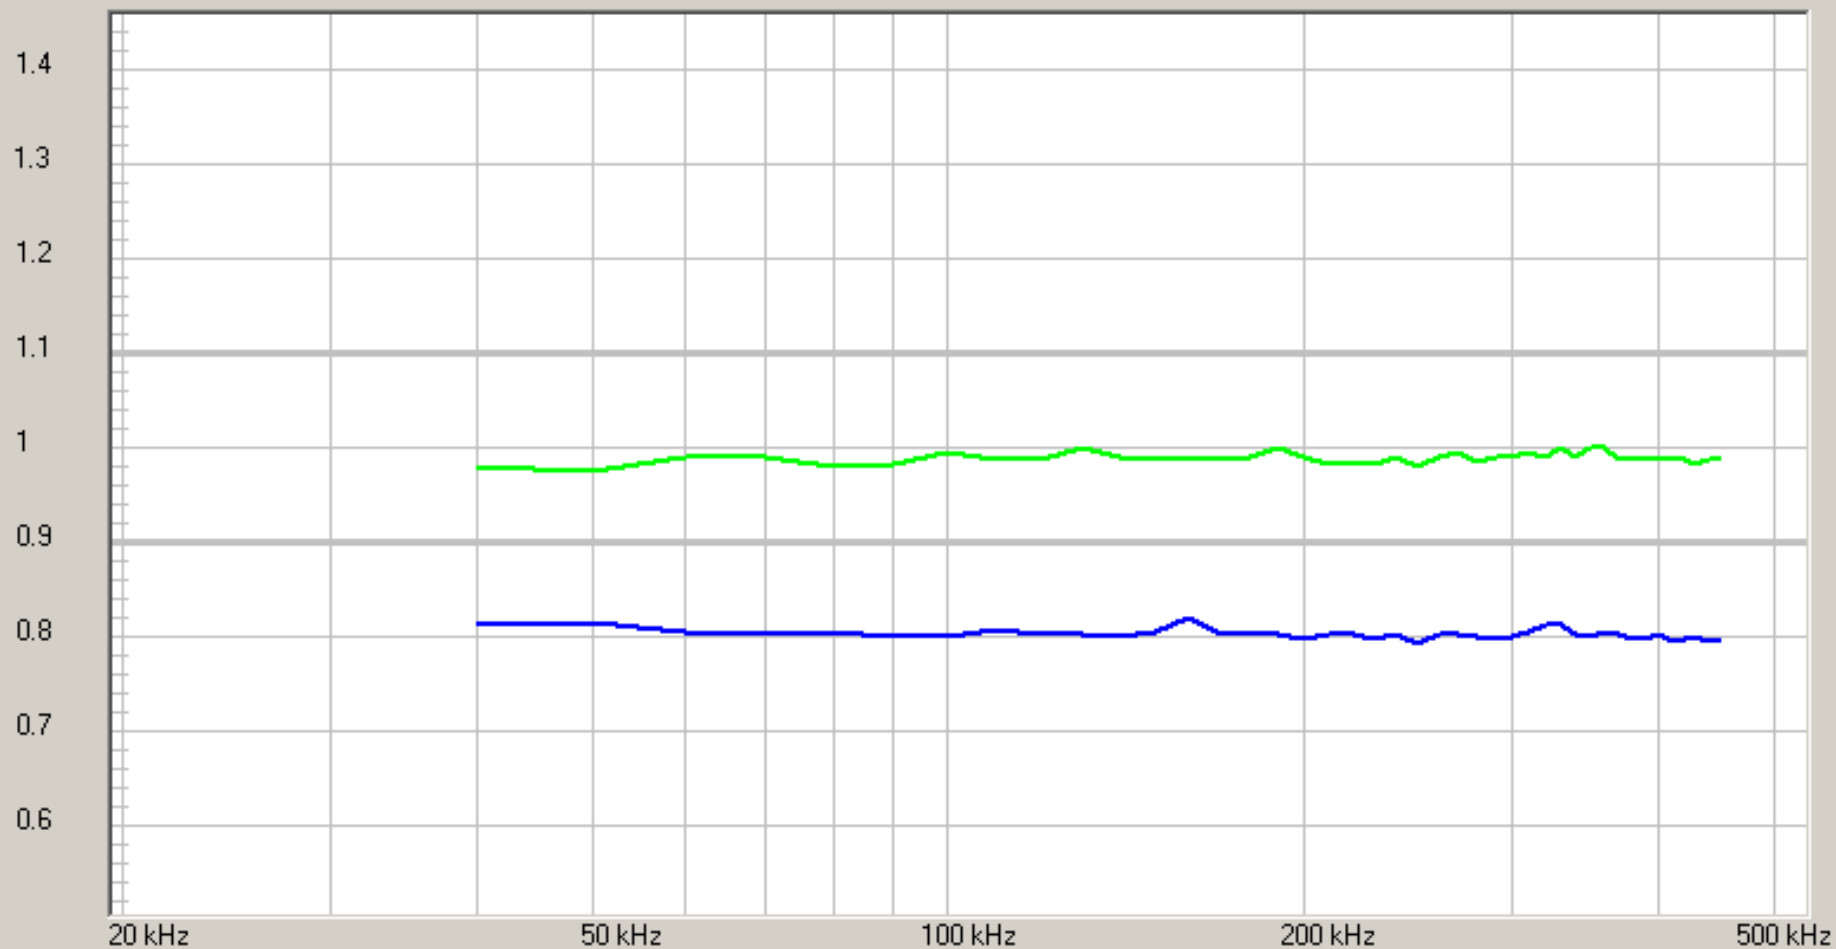

Measurement range

40 - 450 kHz

Step 10 kHz

- Symmetry +  
 Symmetry -

Single measurement

100 kHz

Send

Symmetry Test

Start

Results

50 kHz --> .974  
100 kHz --> .995  
150 kHz --> .987  
200 kHz --> .991  
250 kHz --> .981  
300 kHz --> .99

Comments

DuT Sample Slave

Symmetry not OK  
Symmetry OK